Odin Metrology Inc.
Calibration of Brüel & Kjær Instruments
Thousand Oaks, CA 91320 (805) 375-0830

Measurement of Filter Response BRÜEL & KJÆR Analyzer

TYPE 2133 **s/n** 1583224

Tolerances are per ***Class 1 IEC 1260, 1995*** (indicated with solid lines)

1/3 Octave Band Filter center Frequency : 1000.00 **Hz**

channel A ***JAN 02, 2001***

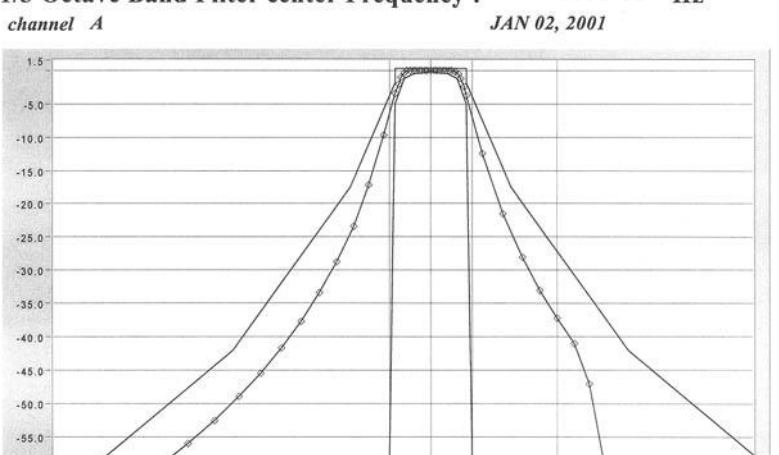

Relative Frequency f/fm (log scale)

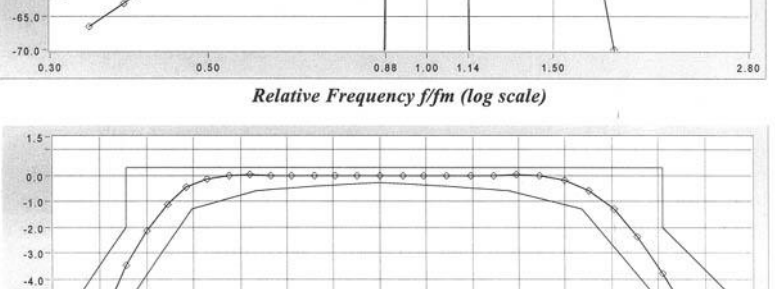

Relative Frequency f/fm